

IMAGES IN INTERVENTION

Comprehensive Imaging of Coronary Stent Using Ultra-High Resolution Spectral Photon Counting CT

A Multimodality Validation

Guillaume Fahrni, MD,^{a,b,c} Sara Boccalini, MD, PhD,^{a,b} Cyril Prieur, MD,^d Philippe Douek, MD, PhD,^{a,b} Salim A. Si-Mohamed, MD, PhD^{a,b}

The recent clinical introduction of ultra-high-resolution spectral photon-counting computed tomography (SPCCT) has opened new frontiers in coronary stent imaging.^{1,2} A 66-year-old man known for previous left anterior descending coronary artery (LAD) stent implantation was admitted to the emergency department of our institution with suspected non-ST-segment elevation acute coronary syndrome. Invasive coronary angiography (ICA) including optical coherence tomography demonstrated a 60% intrastent restenosis in the proximal LAD, which was due to a focal suboptimal stent expansion (Figures 1A and 1B). Diffuse intrastent neointimal hyperplasia and a mid-LAD gap between 2 stents were also identified. The initial treatment was conservative with medical therapy for 1 month, but repeat ICA showed no evolution of the stenosis. As the fractional flow reserve assessment was negative for significant hemodynamic stenosis, with 2 measurements of 0.87 and 0.86, no intervention was planned. As part of our research protocol, 2 coronary computed tomographic angiographic examinations were performed 1 day prior to repeat ICA, using a clinically available computed tomographic

scanner (CT 7500, Philips Healthcare; 0.625-mm³ resolution) and a clinical research prototype spectral photon-counting computed tomographic scanner in ultra-high-resolution mode (Philips Healthcare; 0.25-mm³ resolution). Although both systems identified the 60% intrastent stenosis in the proximal LAD, SPCCT enabled better stent structure characterization, with improved visualization of the focal suboptimal stent expansion that was due to compressive coronary calcifications (Figures 1E and 1H), as well as better characterization of the diffuse neointimal hyperplasia and the mid-LAD stent gap, which was initially missed on conventional computed tomography (Figures 1F and 1I).

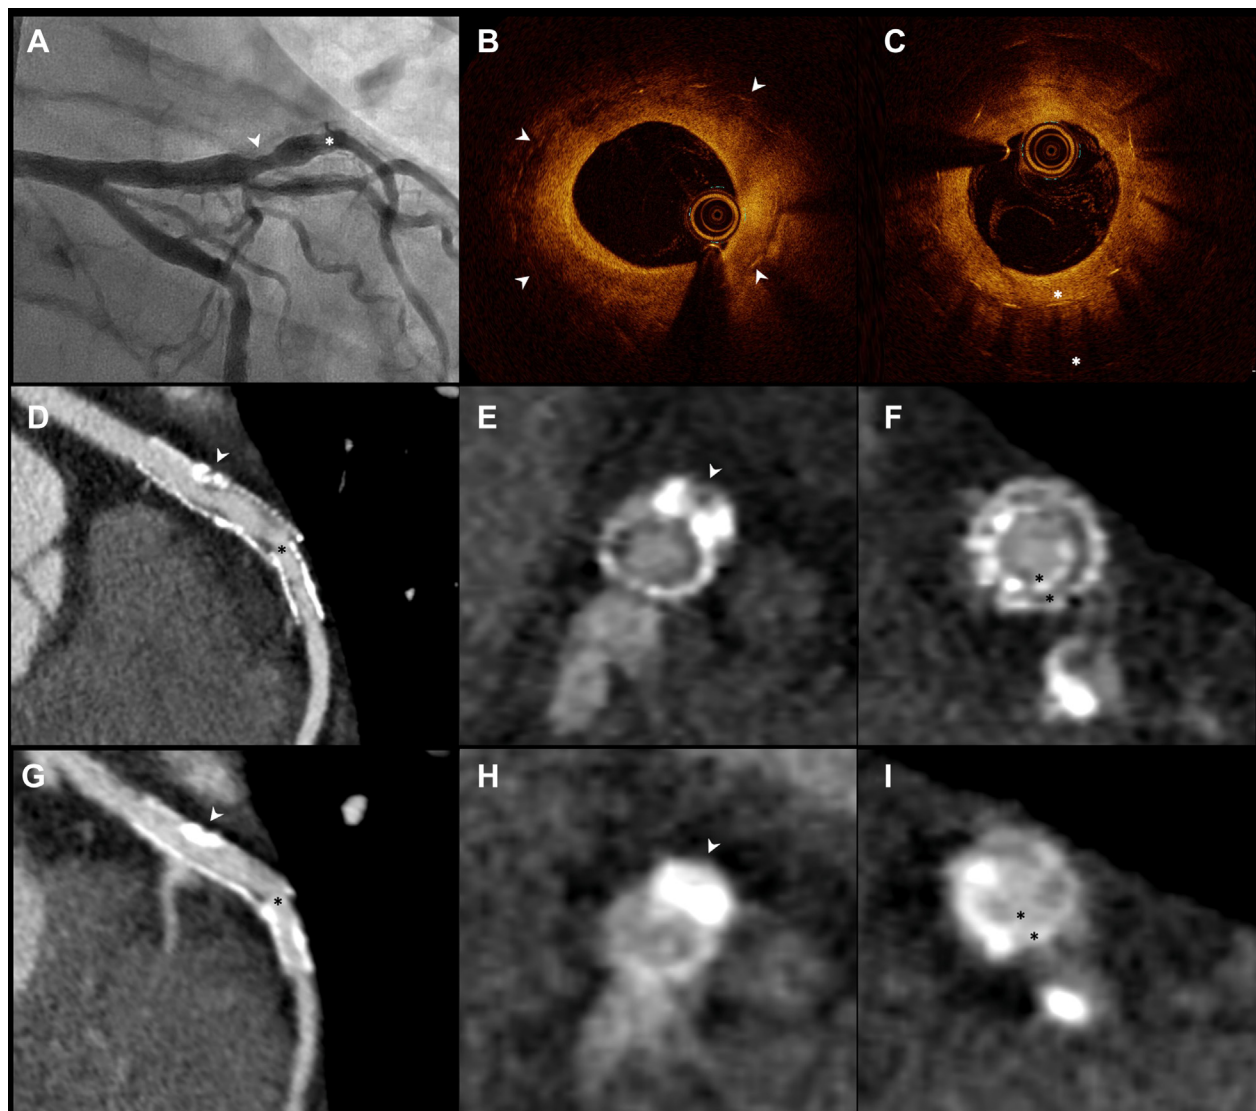
SPCCT has the potential to allow a comprehensive noninvasive imaging assessment of coronary stents, whereas conventional computed tomography struggles because of lesser spatial resolution and significant metallic artifacts limiting image quality.

ACKNOWLEDGMENTS The authors thank Hugo Lacombe, Angèle Houmeau, Morgane Bouin, Apolline Barbe, and Marjorie Villien for their help in image reconstruction, patient management, and project collaboration.

From the ^aUniversity Lyon, INSA-Lyon, University Claude Bernard Lyon 1, UJM-Saint Etienne, CNRS, Inserm, CREATIS UMR 5220, U1206, Villeurbanne, France; ^bDepartment of Radiology, Hôpital Louis Pradel, Hospices Civils de Lyon, Bron, France; ^cCardiothoracic and Vascular Division, Department of Diagnostic and Interventional Radiology, Lausanne University Hospital and University of Lausanne, Lausanne, Switzerland; and the ^dDepartment of Cardiology, Hôpital Louis Pradel, Hospices Civils de Lyon, Bron, France.

The authors attest they are in compliance with human studies committees and animal welfare regulations of the authors' institutions and Food and Drug Administration guidelines, including patient consent where appropriate. For more information, visit the [Author Center](#).

Manuscript received July 4, 2023; accepted July 25, 2023.

FIGURE 1 Comprehensive Imaging of Coronary Stent and Its Complications Using Ultra-High Resolution Spectral Photon-Counting CT

Right anterior oblique invasive coronary angiography (ICA) (**A**), optical coherence tomography (OCT) (**B, C**), spectral photon-counting computed tomography (SPCCCT) (**D-F**), and conventional computed tomography (CT) (**G-I**) of the proximal and mid-LAD. The 60% proximal intrastent restenosis due to a focal suboptimal stent expansion (**arrowheads** in **A** and **B**) detected on ICA and OCT was explained by a compressive external calcification (**arrowheads** in **D, E, G**, and **H**) that was best characterized on SPCCCT. The distal stent gap (**asterisks**) was initially missed on conventional CT but was visible on SPCCCT. Note the diffuse intrastent neointimal hyperplasia that is also better visible with SPCCCT.

FUNDING SUPPORT AND AUTHOR DISCLOSURES

This work was supported by European Union Horizon 2020 grant 643694. Dr Fahrni is supported by a research grant from the Swiss Society of Radiology and Lausanne University Hospital. The authors have reported that they have no relationships relevant to the contents of this paper to disclose.

ADDRESS FOR CORRESPONDENCE: Dr Salim Si-Mohamed, CHU Cardiologique Louis Pradel, Department of Cardiovascular and Thoracic Radiology, 59 Boulevard Pinel, 69500 Bron, France. E-mail: salim.si-mohamed@chu-lyon.fr.

REFERENCES

1. Si-Mohamed S, Boccalini S, Lacombe H, Bousset L, Greffier J, Douek PC. Coronary CT angiography with photon-counting computed tomography: first-in-human results. *Radiology*. 2022;303(2):303-313. <https://doi.org/10.1148/radiol.211780>
2. Boccalini S, Si-Mohamed SA, Lacombe H, et al. First in-human results of computed tomography angiography for coronary stent assessment with a spectral photon counting computed tomography. *Invest Radiol*. 2021;57(4):212-221. <https://doi.org/10.1097/RLI.0000000000000835>

KEY WORDS coronary artery disease, coronary computed tomography angiography, coronary stent, neointimal hyperplasia, spectral photon-counting computed tomography